


Device specification

Product code	MU-IN-D-8-L
Serial Number	MU-BJ-121-121
H/W Version	01.08
Trip Number	14
Description	Platelets
Battery	OK
Original time zone	GMT -12:00 Daylight time
Start	Friday, 8th May 2009, 4:50:30 PM
Finish	Friday, 8th May 2009, 4:58:45 PM
Sampling	5 seconds
Readings	100 (8 minutes, 15 seconds)
Active	-40.0 to 70.0 °C
Specification	20.0 to 25.0 °C

Statistics

Highest	25.6 °C
Average	25.3 °C
Lowest	24.8 °C
High Alarm	Activated
Low Alarm	Not activated

Record

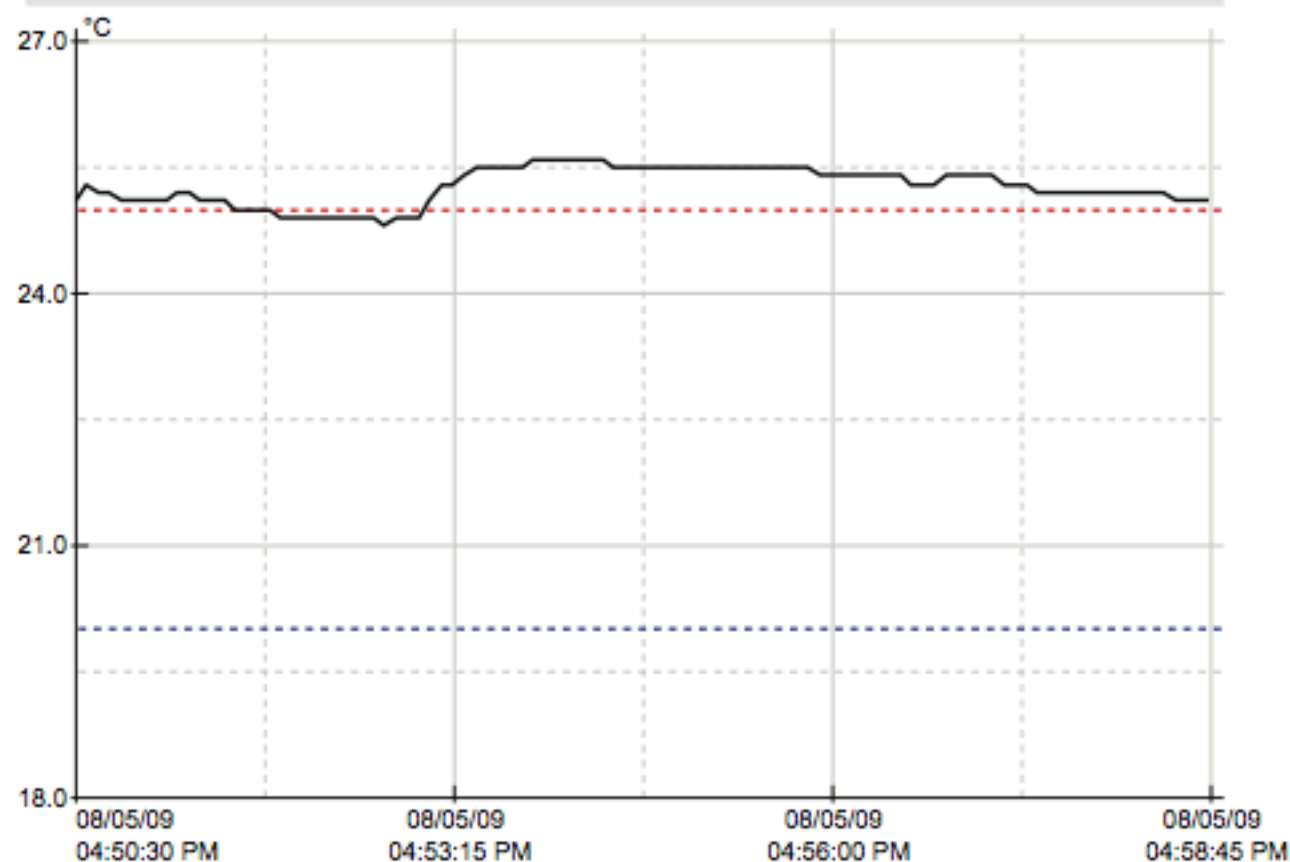

Out of specification

25.0 to 35.9 °C	7 minutes, 5 seconds
-----------------	----------------------